



# omnia LH75



# omnia LH75 Pro

Compact benchtop systems designed to meet the automation and efficiency requirements of the molecular biology laboratory

Proven technology to enhance the efficiency of your RNA extraction and PCR set up workflow

## Automation, reliability and flexibility all in one

**Omnia LH 75** and **Omnia LH 75 PRO** are the A.Menarini Diagnostics compact workstations designed to fully automate nucleic acid extraction and PCR plate setup and streamline your laboratory workflow.

The systems allow **full process automation** from primary tubes to a ready-to-go real time PCR plate.

**Operator intervention** is limited to platform set up and to reagent and sample loading. An **onboard**

**barcode reader** automatically identifies samples and reagents.


**Plate set up information is automatically transferred** to the thermal cycler and to the LIS for easy and error-free traceability.

High-quality nucleic acids are obtained rapidly and efficiently by using **best-in-class magnetic bead extraction kits**.

**Omnia LH 75** has a **processing capacity** of up to 24 samples/run and **Omnia LH 75 PRO** of up to 48, VTM tube to PCR plate without manual intervention.



Primary tube handling, the onboard barcode reader and bidirectional connection with the LIS ensure complete traceability

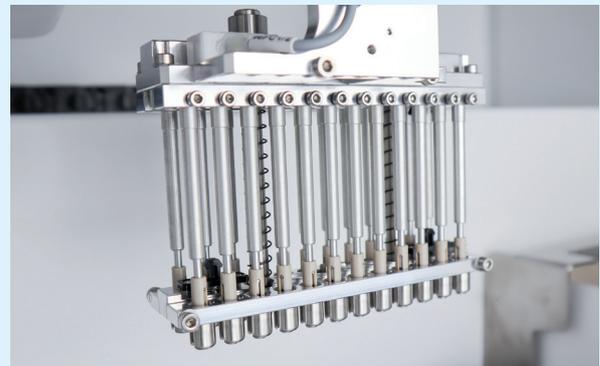

24 magnet rods for parallel magnetic beads management/sample washing steps



Single tip head for dispensing and transfer of liquids




User-friendly interface software with guided procedures ensures minimum operator's effort


# DECK LAYOUT (SBS-COMPLIANT)

1. Barcode scanners
2. Racks for eluate stocking
3. Reagent input rack
4. Sample input racks
5. Temperature-controlled rack
6. Thermoshaker
7. Customizable position
8. PCR setup position
9. Washing plate
10. Tips
11. Removable waste bin
12. Covers for magnets

omnia LH 75 Pro

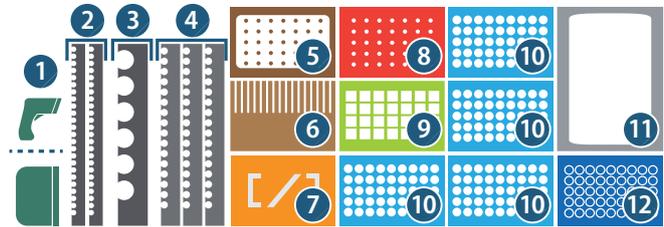

omnia LH 75

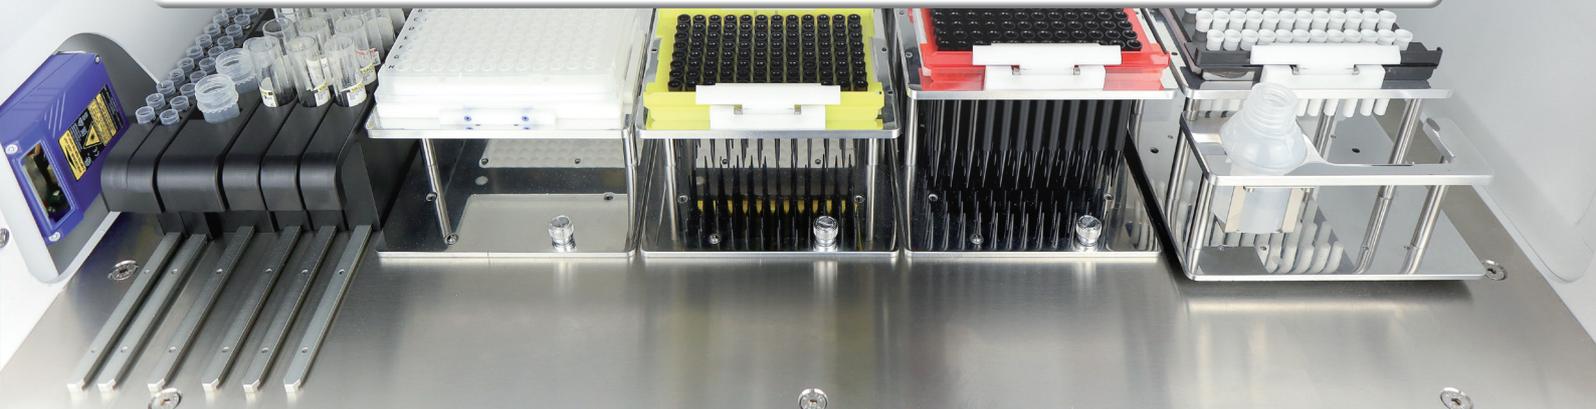

# SUPPORTED COVID APPLICATIONS

**RADI COVID-19  
detection kit**



**CoronaMeltVAR SARS CoV-2  
Real Time PCR kit**



**CoronaVar SARS-CoV-2  
Variant detection kit**



Visit our website for details and updates  
on A.Menarini Diagnostics Real Time PCR kits:  
<https://www.menarindiagnostics.com/en-us/Home/Laboratory-products/COVID-19/Viral-RNA-Detection>



## At a glance

**Extraction method** Magnetic bead transfer: 24 parallel magnetic rods, for rapid processing of all washing steps

**Input sample types** VTM/UTM, saliva and other body fluids including viral inactivator

**Reagents** CE IVD and RUO magnetic beads extraction kits, Real Time PCR diagnostic kits for SARS Cov-2 detection and variant identification

**Liquid handling** 1 pipetting channel; pipetting volume range: 1 µl to 1000 µl; precision CV: ≤ 0.2% at full stroke; liquid level sensor

**Processing capacity** Up to 24 samples per run (sample tube to PCR plate) on Omnia LH 75, up to 48 on Omnia LH 75 PRO

**Traceability & Connectivity** 2 barcode scanners (integrated + external), bidirectional interface with LIS, direct connection to the most common thermal cyclers

**User-friendly software** Internal control system and remote monitoring through HMI software and a built-in touchscreen

**Assay flexibility** Up to 4 assays with identical PCR profile on the same extracted RNA. Compatible with validated kits and custom assays

**Safety and decontamination** Easy-to-clean deck, UV-lamp (254 nm), removable waste bin, filter tips and disposable components

## Technical Specifications

Power input	xxxxxxx
Power consumption	xxxxxxx
Operating temperature	xxxxxxx
Dimension (WxDxH)	91,6x78,9x84,8 cm
Weight	xxxxxxx
Relative humidity	xxxxxxx
Marking CE-IVD	CE-IVD

## List of products and codes

xxxxxxx	xxxxxxx
xxxxxxx	xxxxxxx